


TECHNICAL DATA

Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

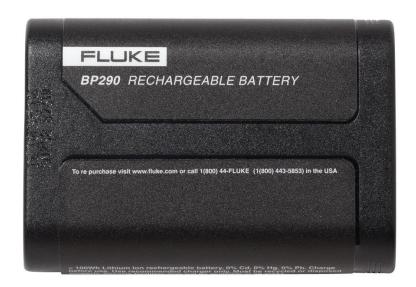

Key features

- 2400 mAh rechargeable Li-ion battery
- Compatible with ScopeMeter® 190 Series III, 190 Series II, 120B Series, MDA-500 Series Motor Drive Analyzers and 430-II Series Power Quality Analyzers

Product overview: Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

The Fluke BP290 Li-ion Battery is a standard capacity battery for use in Fluke 190 Series II and Series III ScopeMeter Test Tools, 120B Series ScopeMeter Test Tools, MDA-500 Series III Motor Drive Analyzers and 430-II Series Power Quality Analyzers. BP290 Li-ion batteries include a charge-status indicator so you can quickly and easily verify charge status in the field, and may be charged either in the instrument itself, or using the option EBC290 External Charger. For situations requiring longer battery operating time consider the Fluke BP291 4800 mAh High Capacity Li-Ion Battery.



Specifications: Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

| Baery | Li-ion, 10.8 V, 2500 mAh, 27 Wh configuration 3ICR19/66 |
|---------------------------------|--|
| Safety | Pollution degree 2 |
| Operating temperature | 0 °C to +50 °C (charging may slow or stop at environmental temperatures >40 °C) |
| Storage temperature | -20 °C to +60 °C |
| Recommended storage temperature | <35 °C |
| Humidity | 0 °C to 10 °C noncondensing 10 °C to 30 °C @ 95 % (±5 %) rh 30 °C to 40 °C @ 75 % (±5 %) rh |
| Altitude | 3000 m |
| Weight | 175 g |
| Dimensions | 22 mm x 85 mm x 59 mm |



Ordering information



Fluke BP290

2400 mAh High Capacity Li-Ion Battery for Fluke 190-series II



Fluke. Keeping your world up and running.®

Fluke (UK) Ltd.
52 Hurricane Way
Norwich, Norfolk
NR6 6JB
United Kingdom
Tel.: +44 (0)20 7942 0708
E-mail: cs.uk@fluke.com
www.fluke.com/en-gb

©2025 Fluke Corporation. All rights reserved. Data subject to alteration without notice. 03/2025

Modification of this document is not permitted without written permission from Fluke Corporation.