


Data teknis

7196B LN₂ Comparison Calibrator



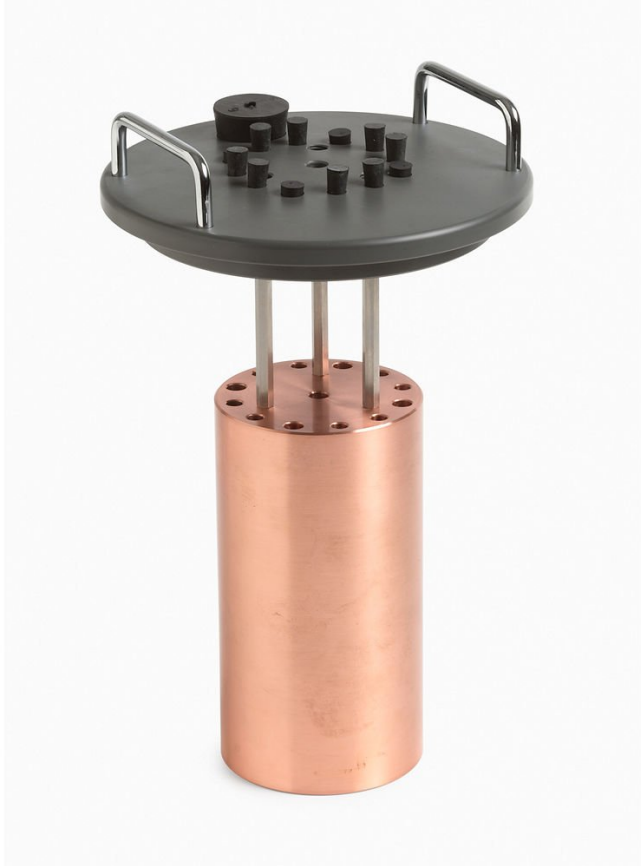

Fitur utama

- Provides low-cost calibrations to -196°C .
- Uncertainty less than 2 mK, ensuring precise and reliable results.
- Simple and straightforward to use.

Ikhtisar Produk: 7196B LN₂ Comparison Calibrator

The nominal boiling point of nitrogen is -196°C at one atmosphere of pressure. The defining triple point of argon is $-189.3442^{\circ}\text{C}$. While there is a difference between the nominal boiling point of nitrogen and the argon triple point, the difference can be corrected for mathematically, and an uncertainty of less than 2 mK from the actual argon triple point is achievable.

Fluke Calibration's LN₂ Comparison Calibrators consist of a vacuum-sealed stainless steel Dewar Flask, a high-purity copper block, and a precision-fit lid. The dewar is filled with LN₂ and the copper block is suspended in it; an SPRT is inserted into the block and a calibration is performed against your own calibrated SPRT. The **7196B-4** includes four 8-mm (0.32") wells. The **7196B-13** includes five 8-mm (0.32") wells and eight 6.35-mm (0.25") wells.

Fluke Calibration's LN₂ Comparison Calibrators are neither expensive nor complicated to use. If you need supporting data or would like to discuss the theory of operation of an LN₂ Comparison Calibrator, call Fluke Calibration today. (Or come to one of our [calibration training courses](#) and we'll show you.)

Spesifikasi: 7196B LN₂ Comparison Calibrator

Specifications	
Temperature	Nominal -196°C depending on atmospheric pressure
Thermal Wells	7196B-4: four 8 mm (0.32") I.D. wells 7196B-13: five 8 mm (0.32") I.D. wells, eight 6.35 mm (0.25") I.D. wells Both blocks: 275 mm immersion from top of lid to boom of well, 150 mm immersion into copper block
Dimensions (outer diameter x height)	168 mm x 406 mm (6.6 in O.D. x 16 in)
Temperature Stability	Typically better than 2 mK/20 min ^[1]
Temperature Uniformity	<0.0004 °C
Volume	5.47 liters (1.45 gallons)
^[1] The equilibrium temperature will change with the atmospheric pressure ($dT/dp \gg 0.085 \text{ mK/Pa}$). The actual temperature stability depends on atmospheric pressure stability.	

Model



7196B-4

LN₂ Comparison Calibrator, 4 holes

7196B-13

LN₂ Comparison Calibrator, 13 holes

Fluke. *Memastikan aktivitas Anda terus berjalan dan beroperasi.*

Fluke Corporation

PO Box 9090, Everett, WA 98206 U.S.A.

For more information call:

In the U.S.A. (800) 443-5853

In Europe/M-East/Africa

+31 (0)40 267 5100

In Canada (800)-36-FLUKE

From other countries +1 (425) 446-5500

www.fluke.com

BUT. FLUKE SOUTH EAST ASIA PTE LTD

Menera Satu Sentra Kelapa Gading #06-05

Jl. Bulevar Kelapa Gading Kav. LA# No. 1

Summarecon Kelapa Gading

Jakarta Utara 14240

Indonesia

Tel: +62 21 2938 5922

Email: info.asean@fluke.com

www.fluke.com/id

©2025 Fluke Corporation. Specifications subject to change without notice.

04/2025

Modification of this document is not permitted without written permission from Fluke Corporation.